
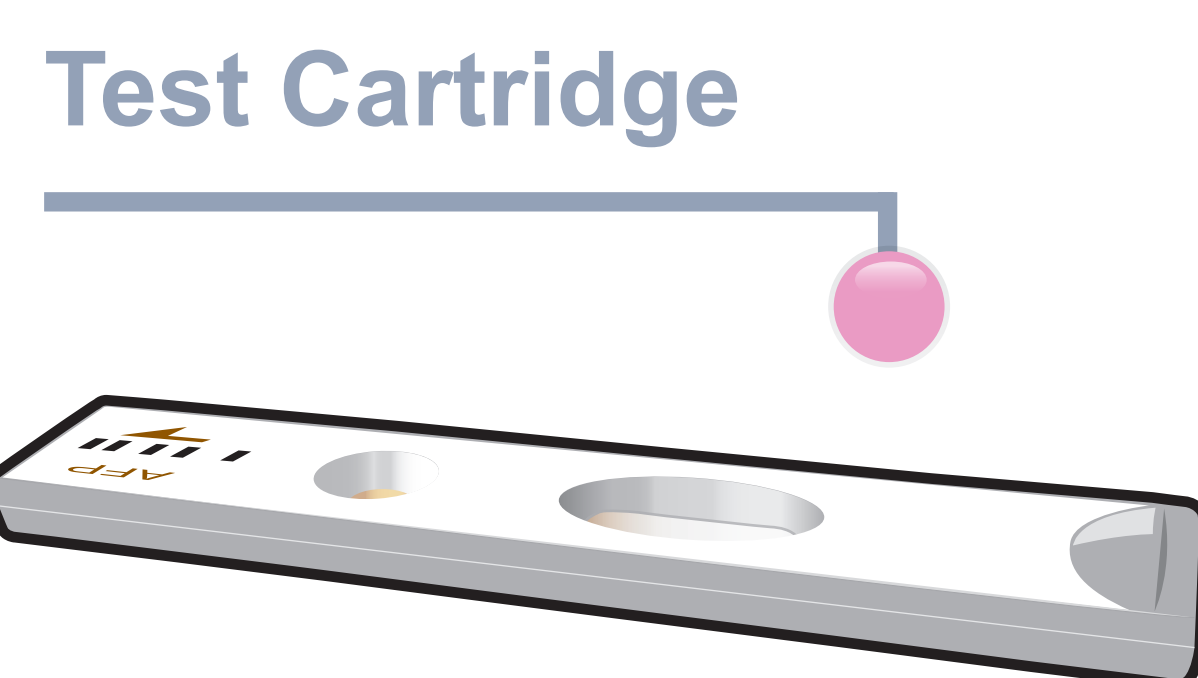
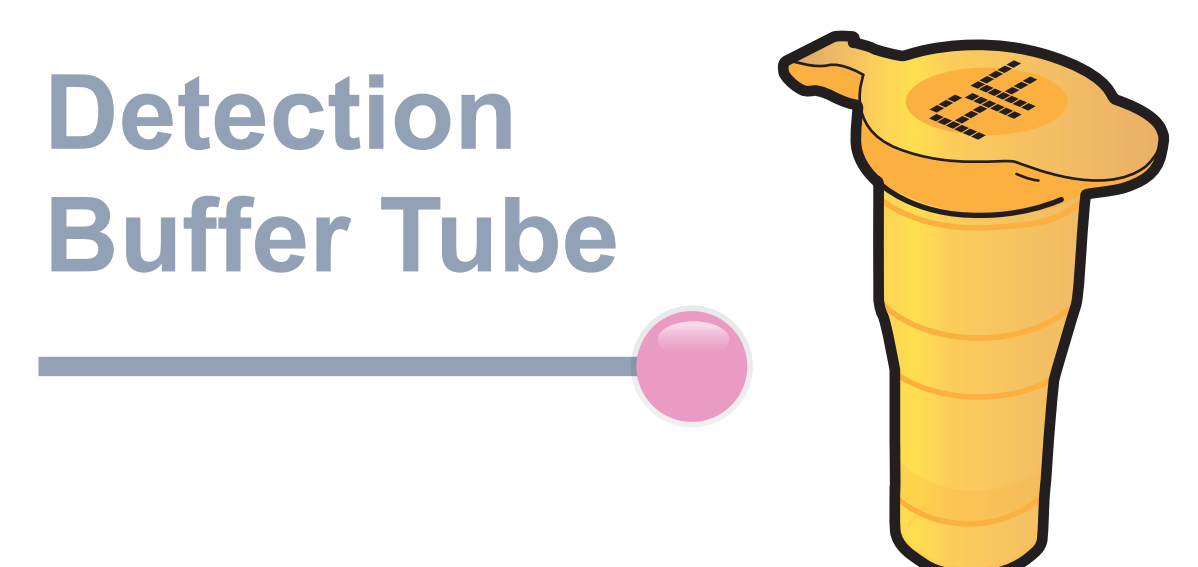


# ichroma<sup>TM</sup> AFP

## Test Setup

### Test Components

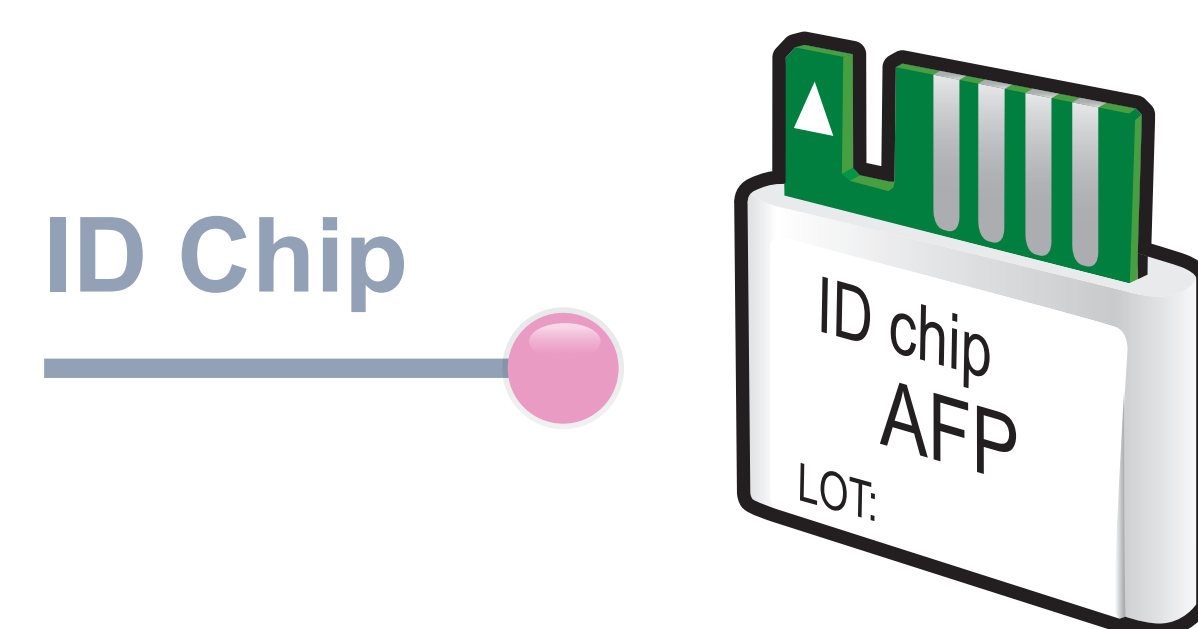

### iCHROMA II Reader




### Important

Allow 'Detection Buffer Tube' to attain room temperature at least for 30 minutes before performing the test

Make sure that lot number of the 'ID Chip' is exactly same as the lot number of 'Test Cartridge' and 'Detection Buffer Tube'


**1** Turn the power switch 'On'

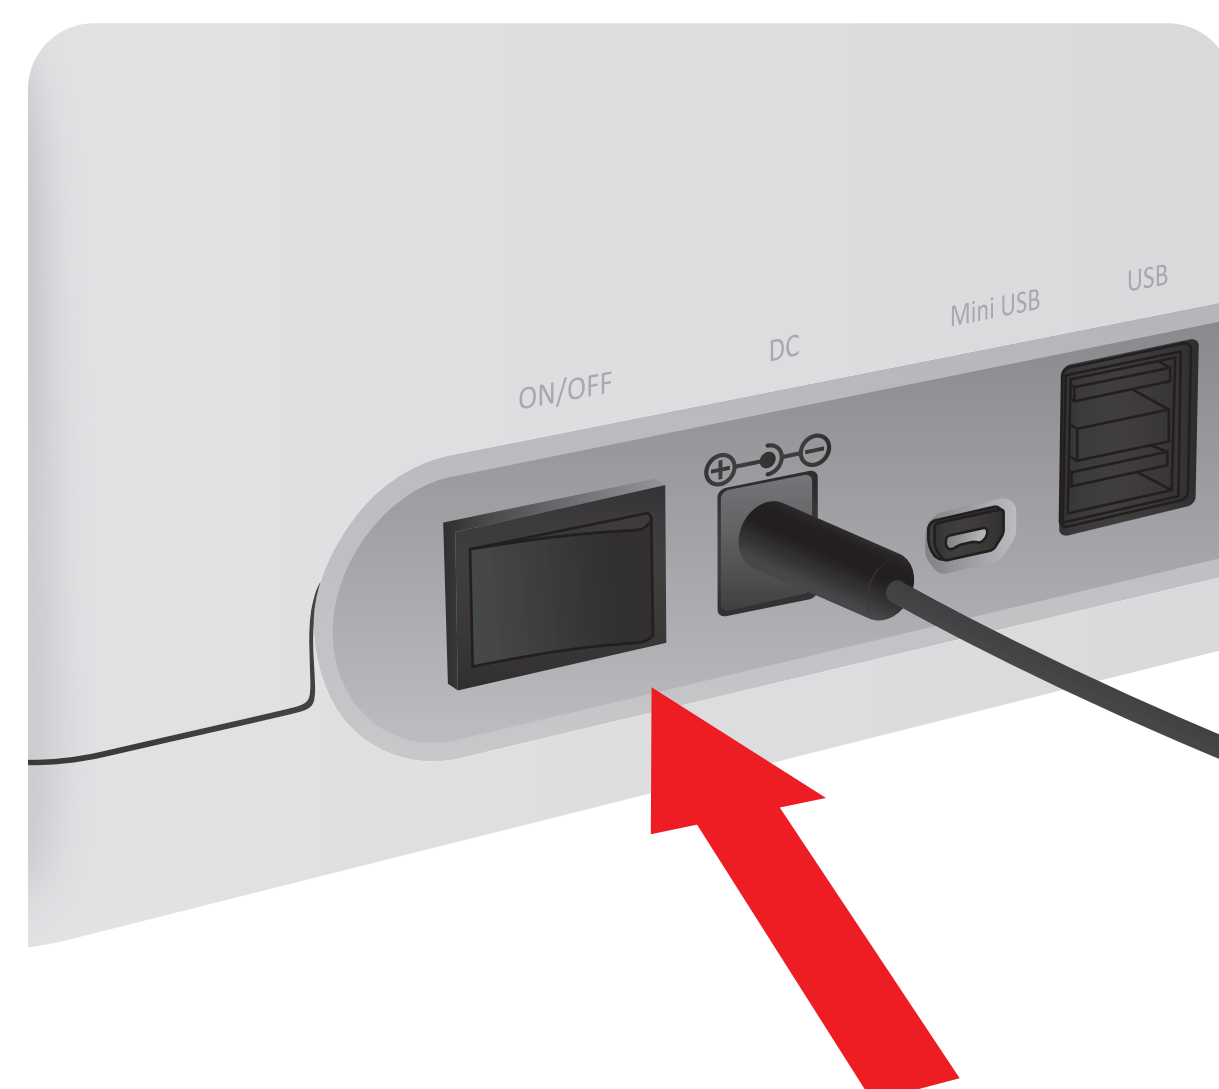

**2** Insert ID Chip




**3** Press 'Multi-test'

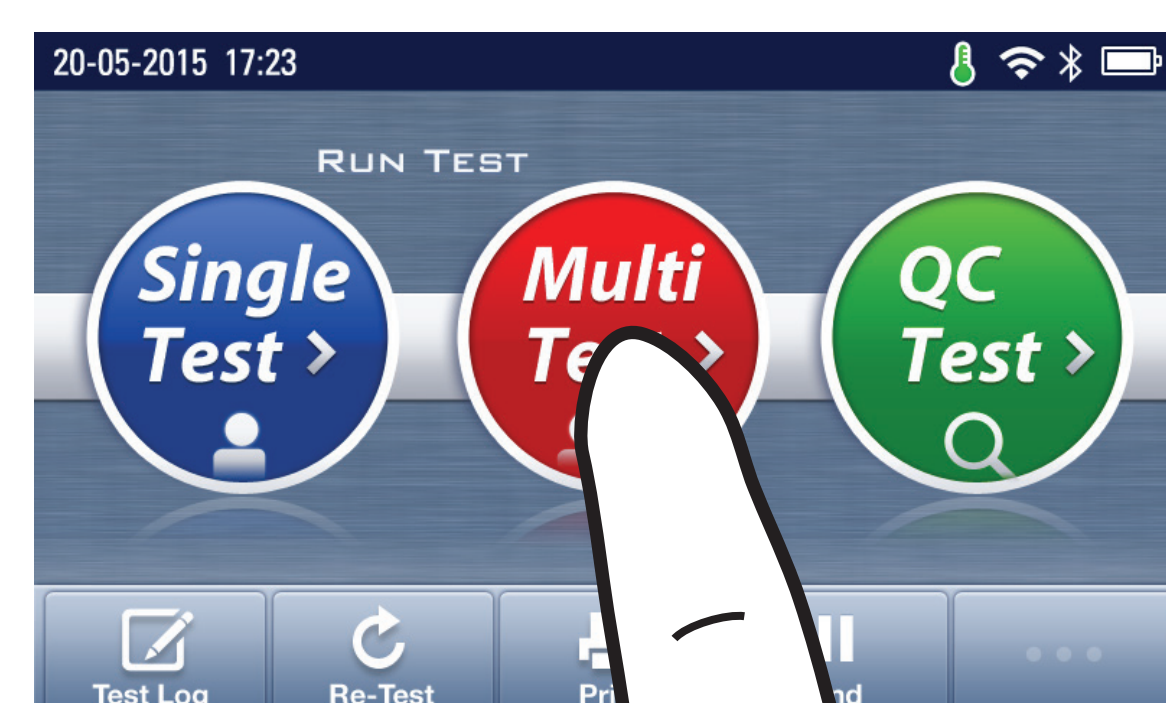

## Test Procedure

### In case of Whole Blood

**1** Draw whole blood

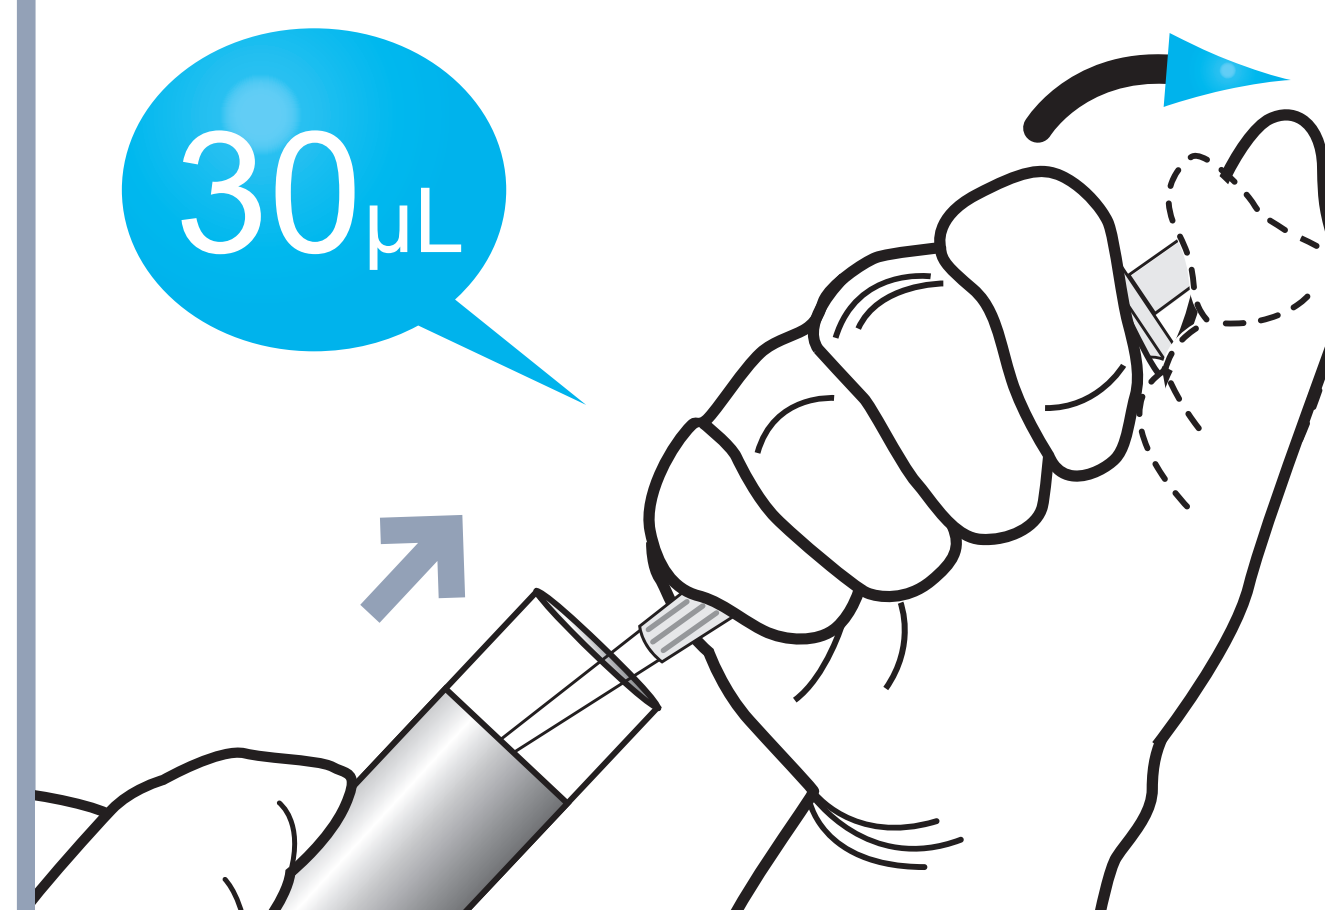

**2** Add it into detection buffer tube



### In case of Serum, Plasma, Control


**1** Draw Serum, Plasma, Control





**2** Add it into detection buffer tube



**3** Shake the detection buffer tube

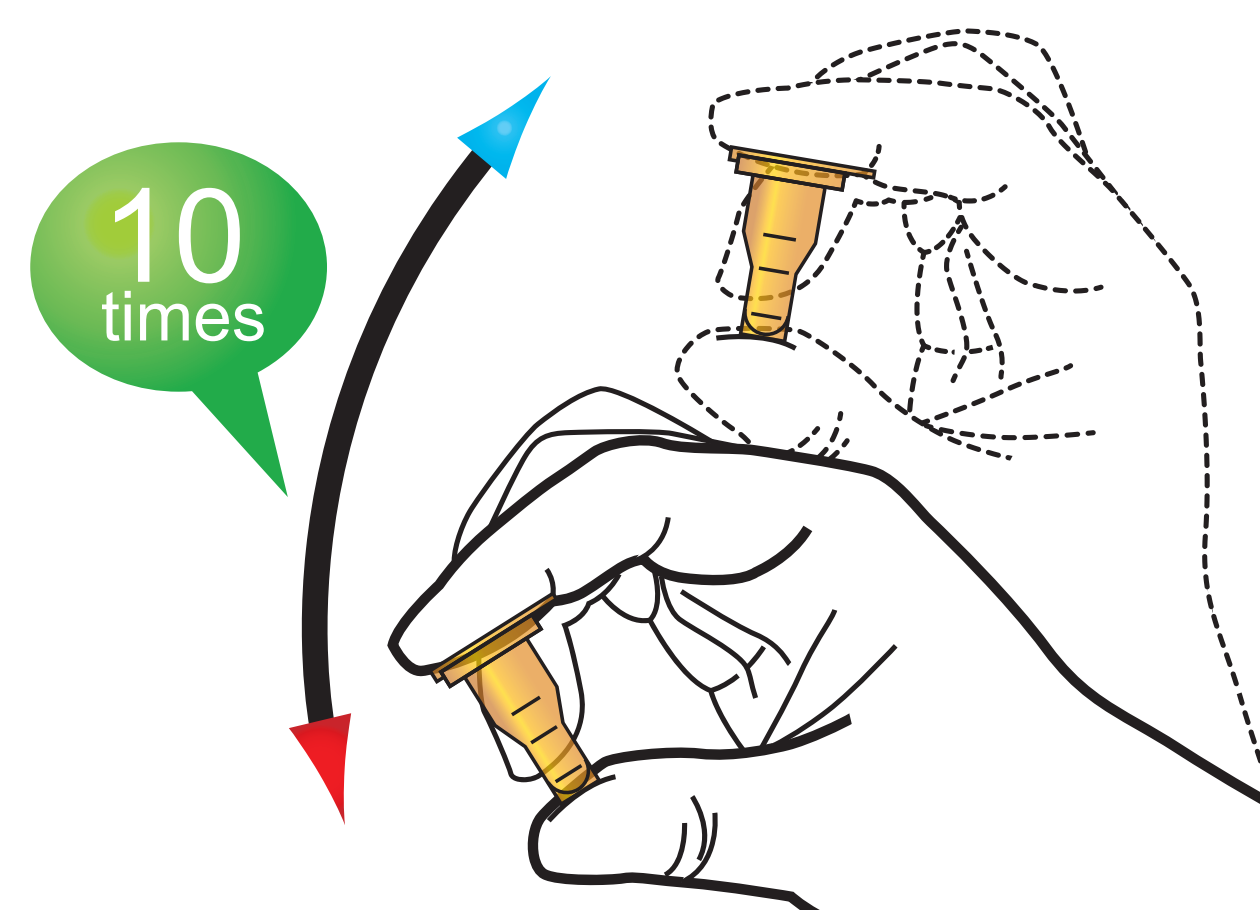

**4** Draw the detection buffer tube

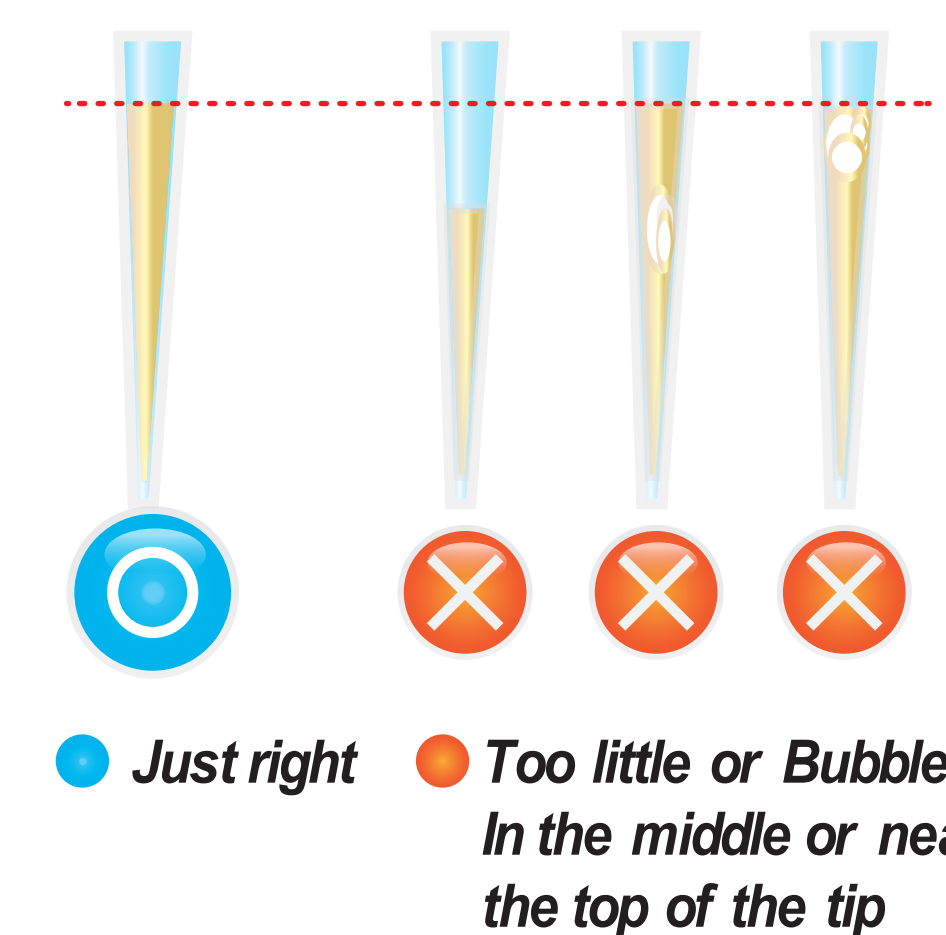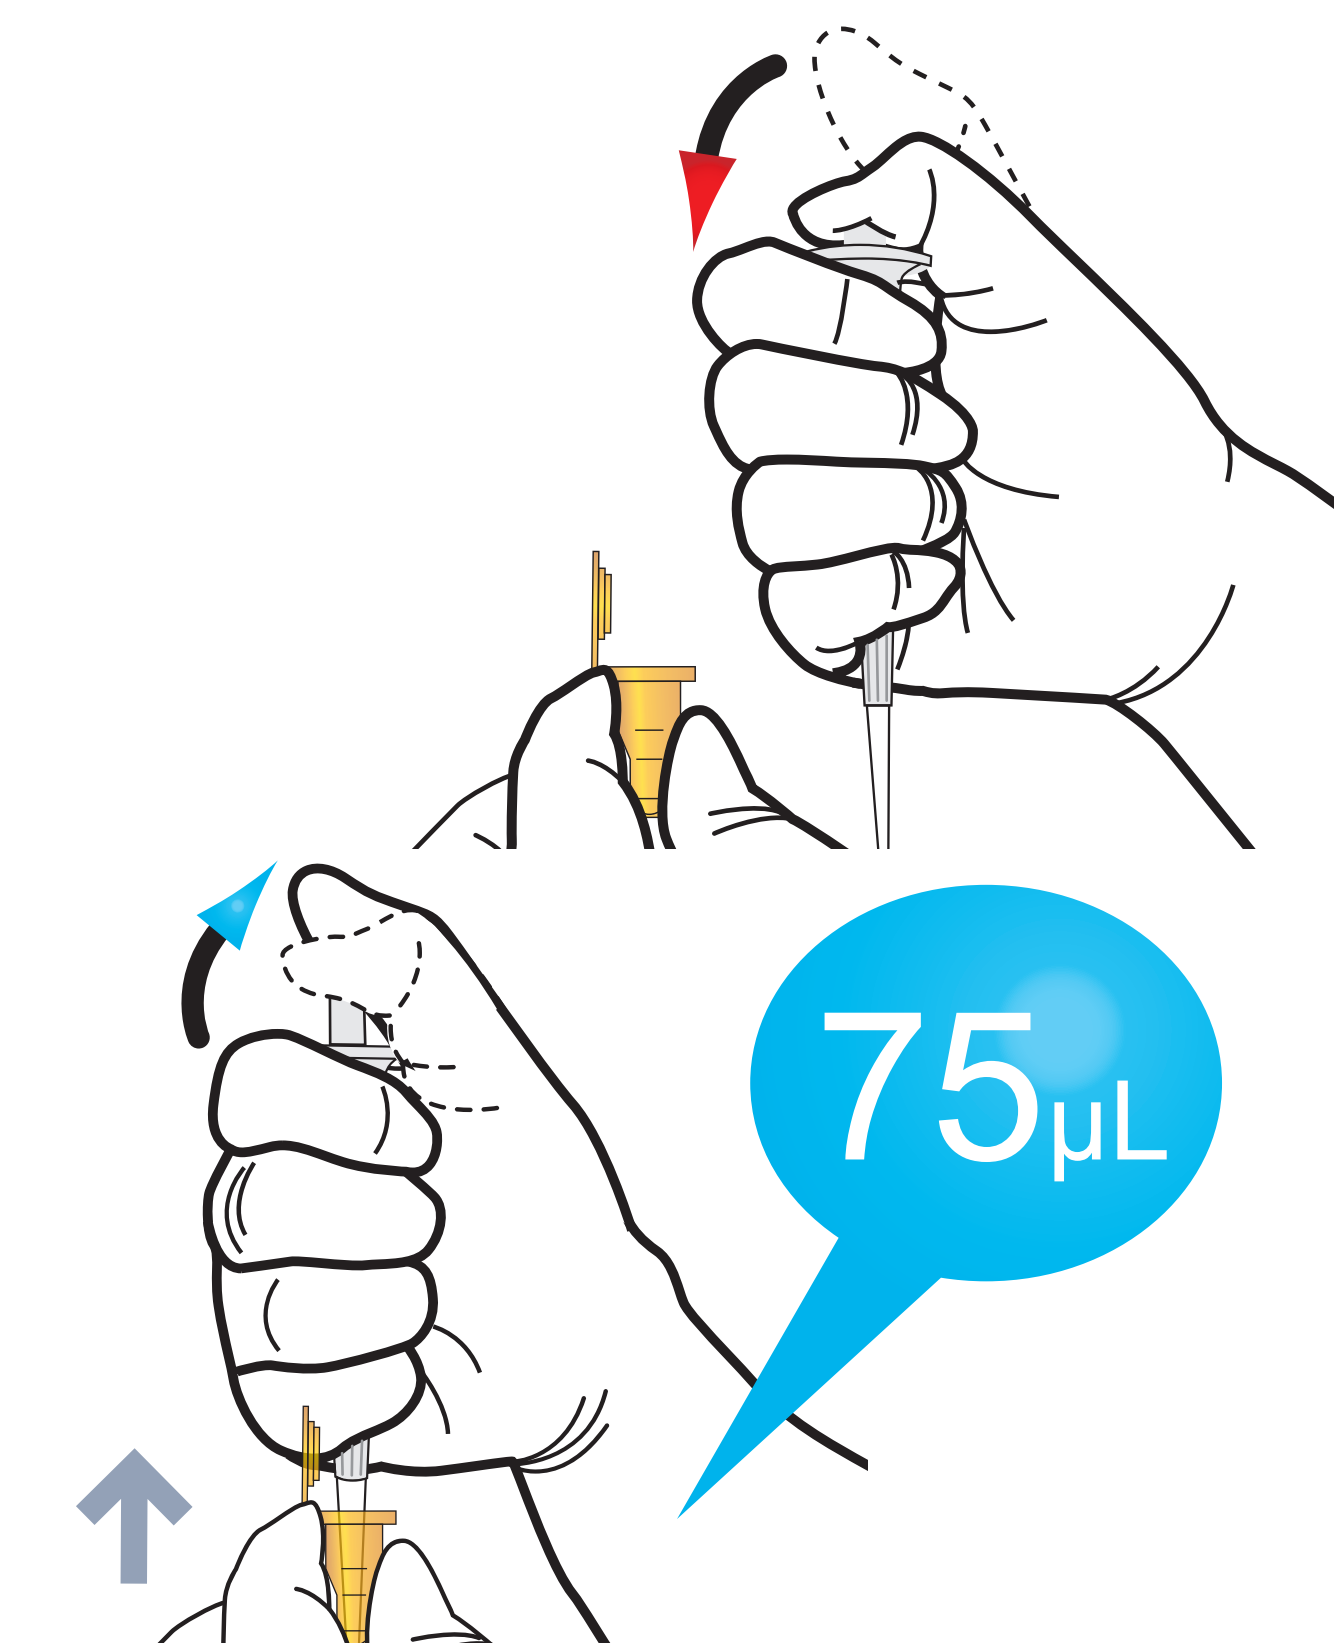

**5** Load the sample mixture




**6** Waiting 15 minutes

**7** Insert the cartridge into ichroma<sup>TM</sup> II Reader



**8** Press 'Select'

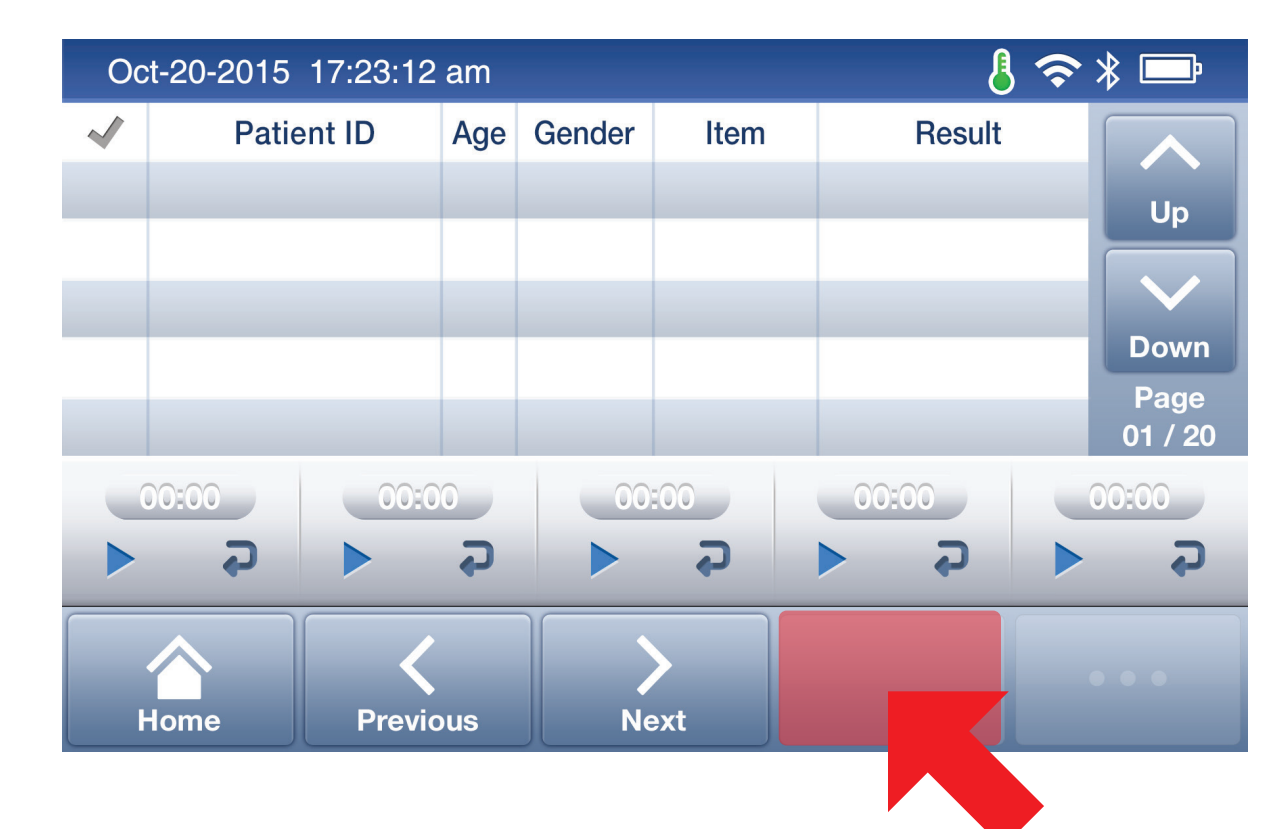

**9** Read the test result



Rev 01\_190325\_AFP