


ichromα™ Cystatin C


Test Setup

Test Components


ID Chip

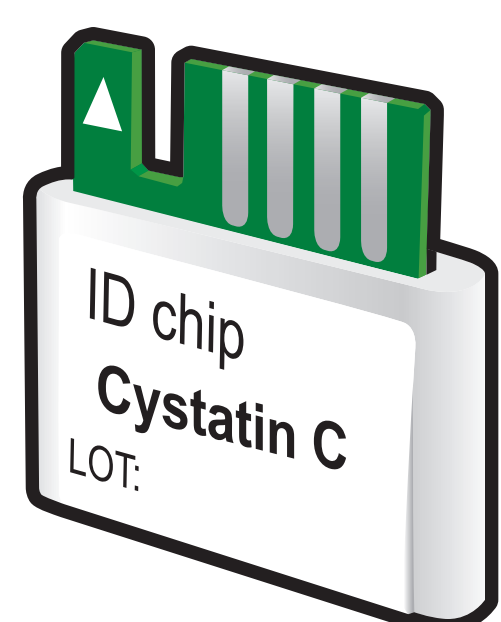

Detection Buffer Tube

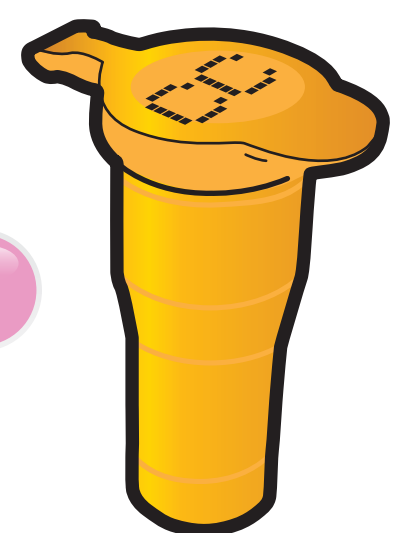

Test Cartridge

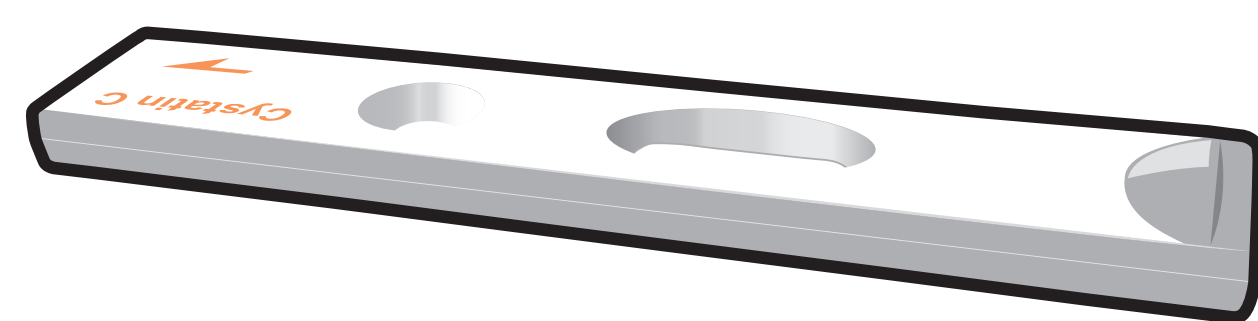

ichromα™ Reader



Important




Allow 'Detection Buffer Tube' to attain room temperature at least for 30 minutes before performing the test




Make sure that lot number of the 'ID Chip' is exactly same as the lot number of 'Test Cartridge' and Detection Buffer Tube


1 Turn the power switch 'On'

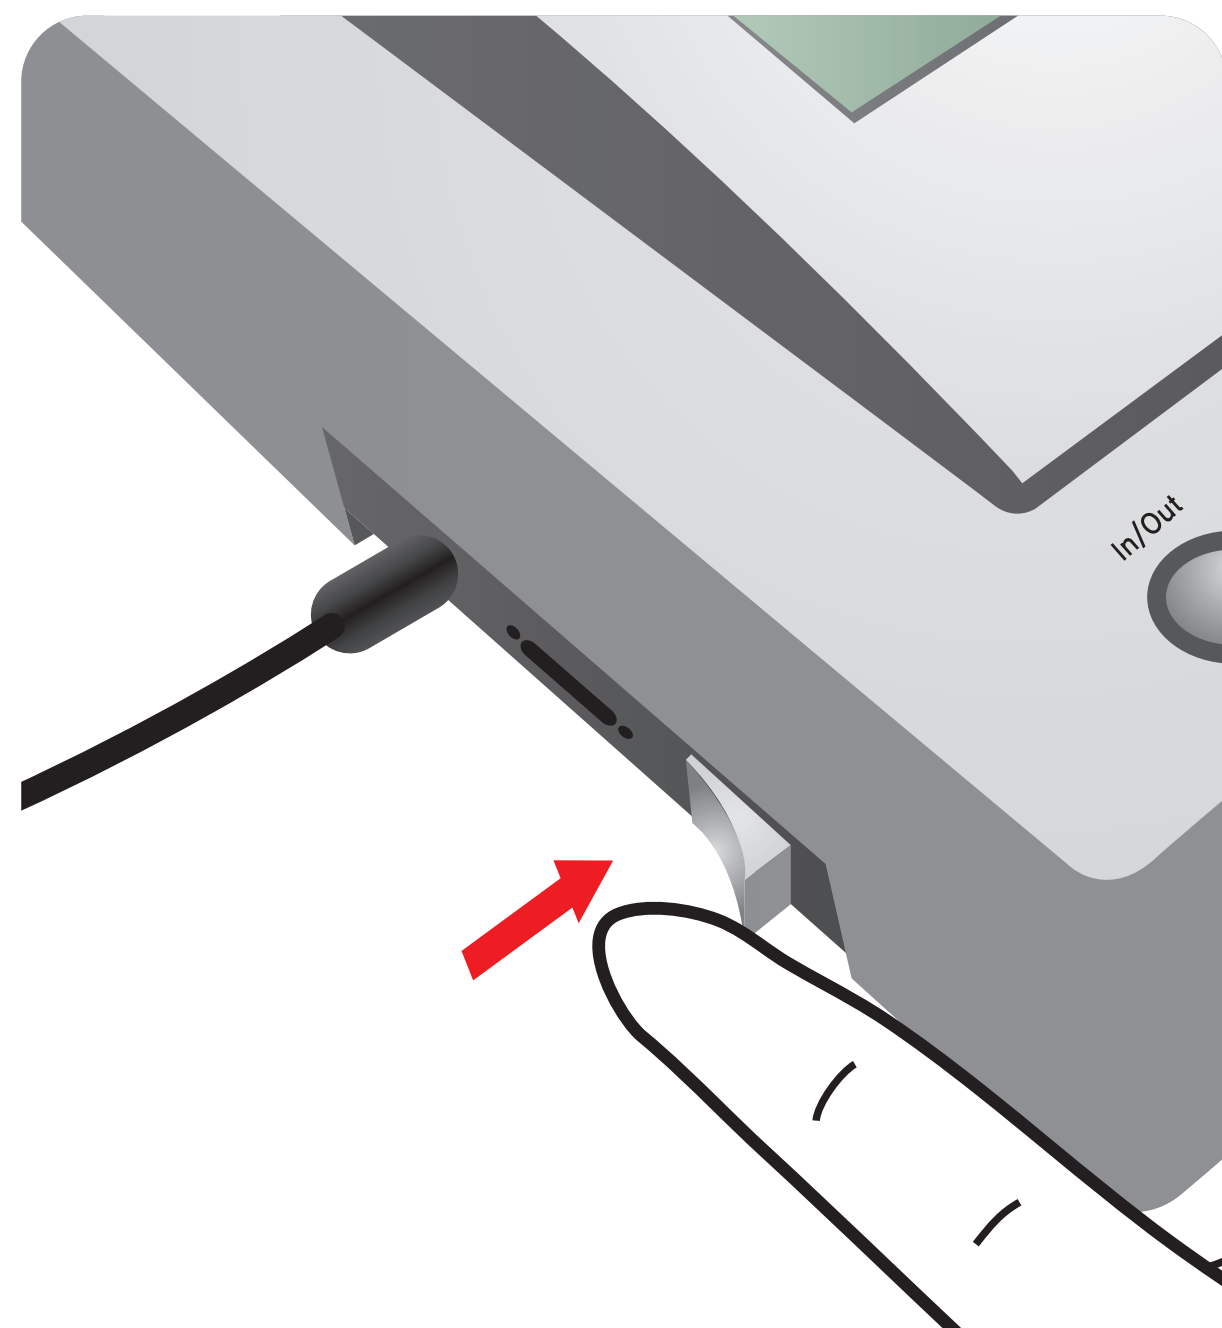

2 Insert ID Chip

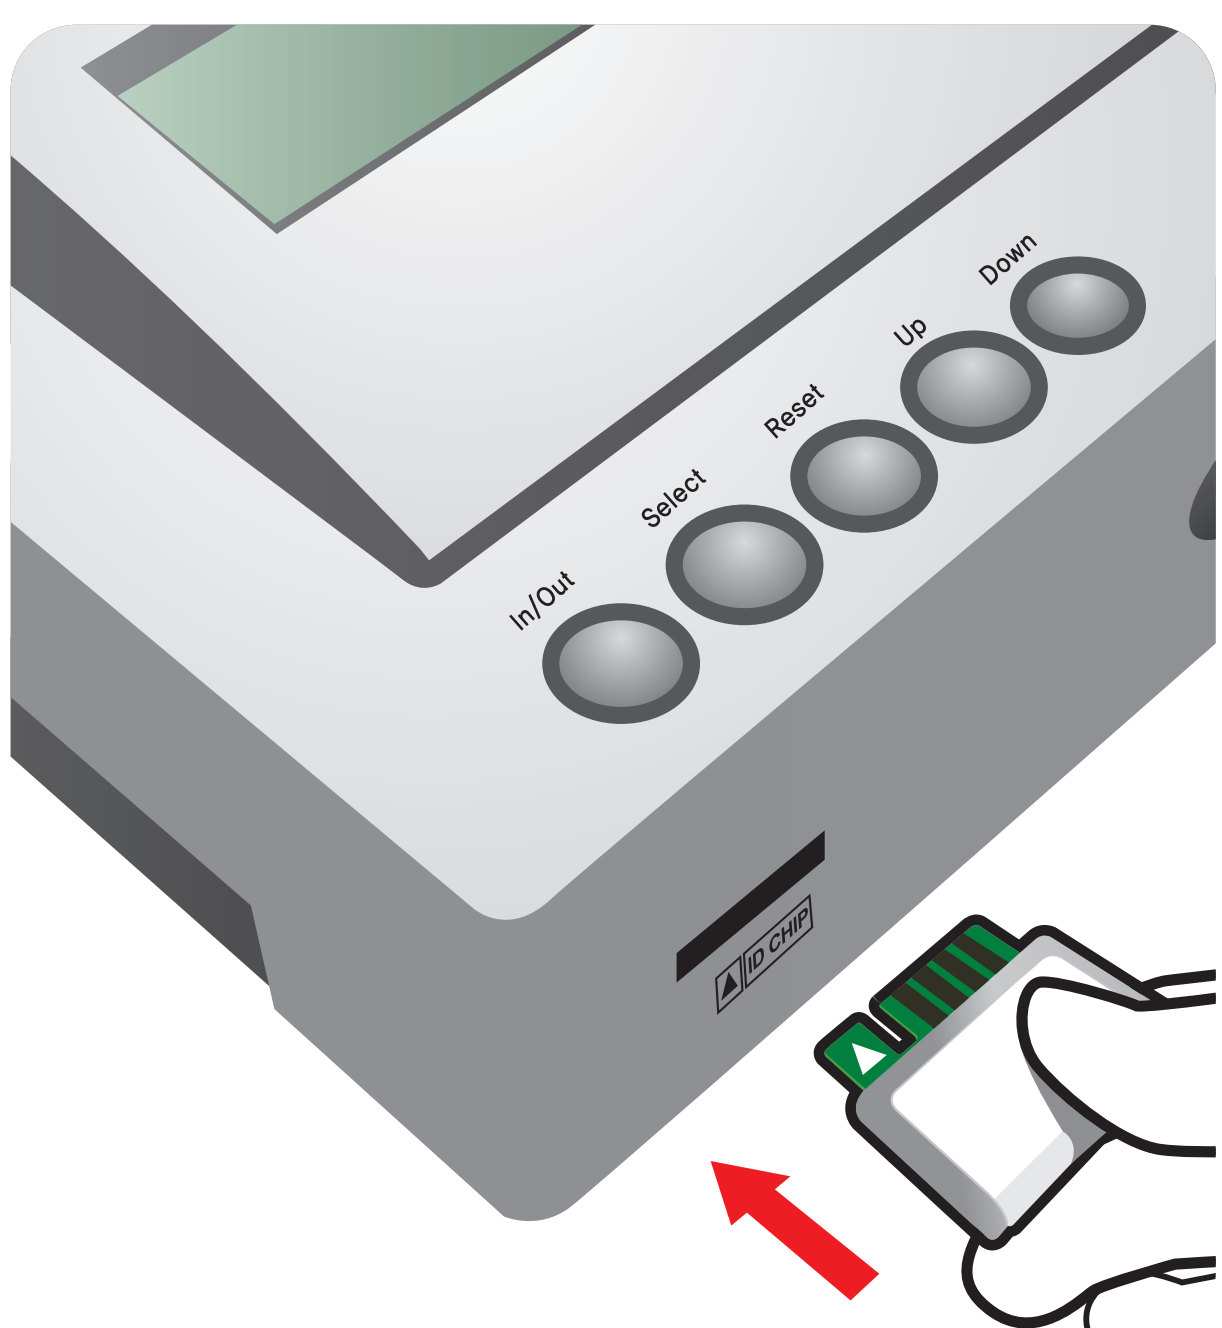

3 Press 'Select'

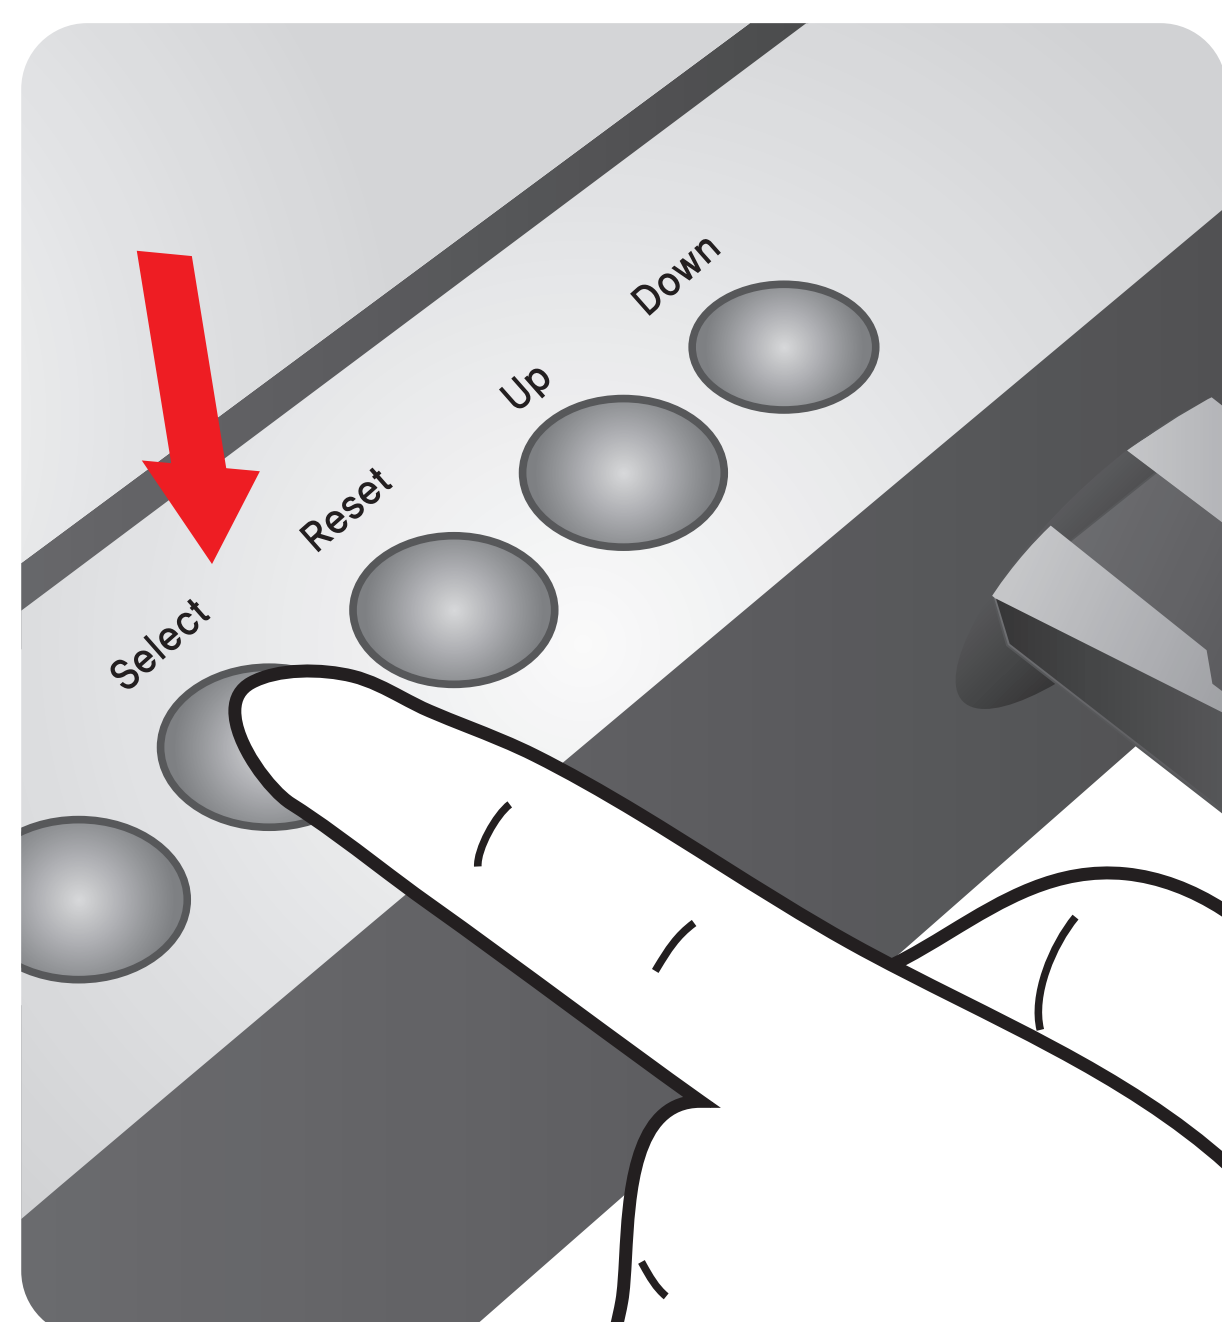


Test Procedure


1 Draw the test sample (Serum or Plasma)



Take 10 µL of with a transfer pipette

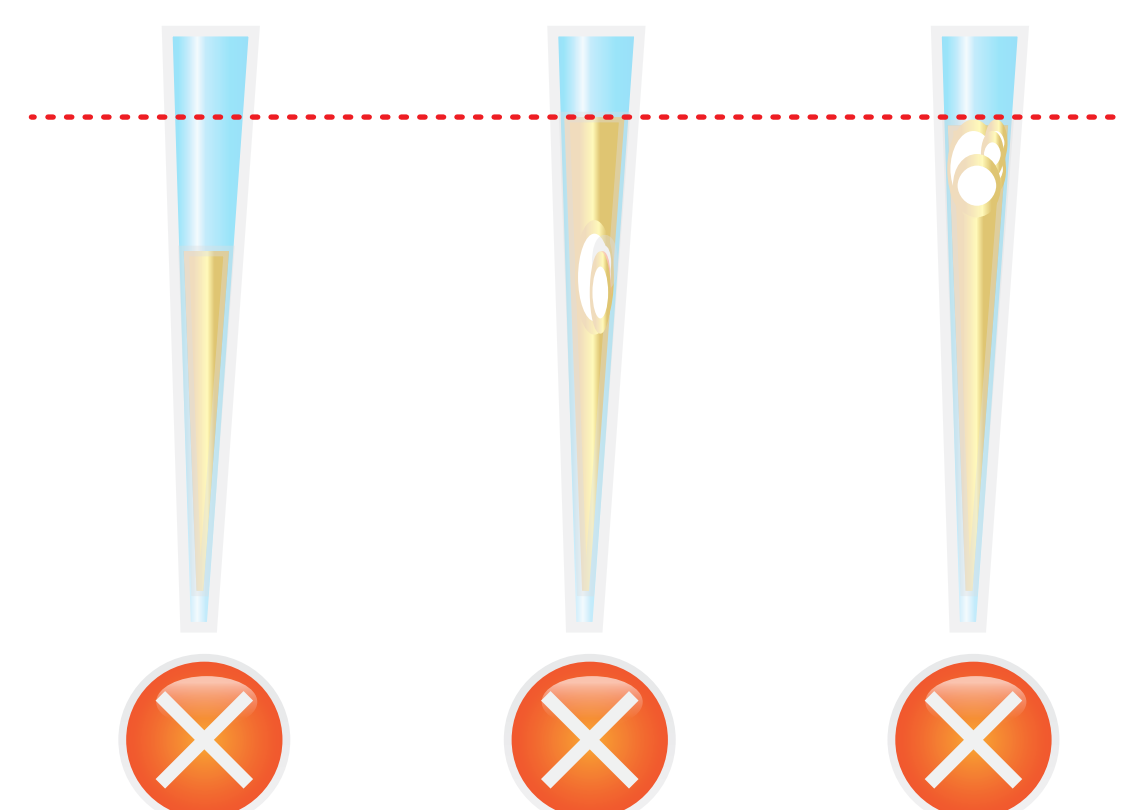


Too little or Bubble in the middle or near the top of the tip

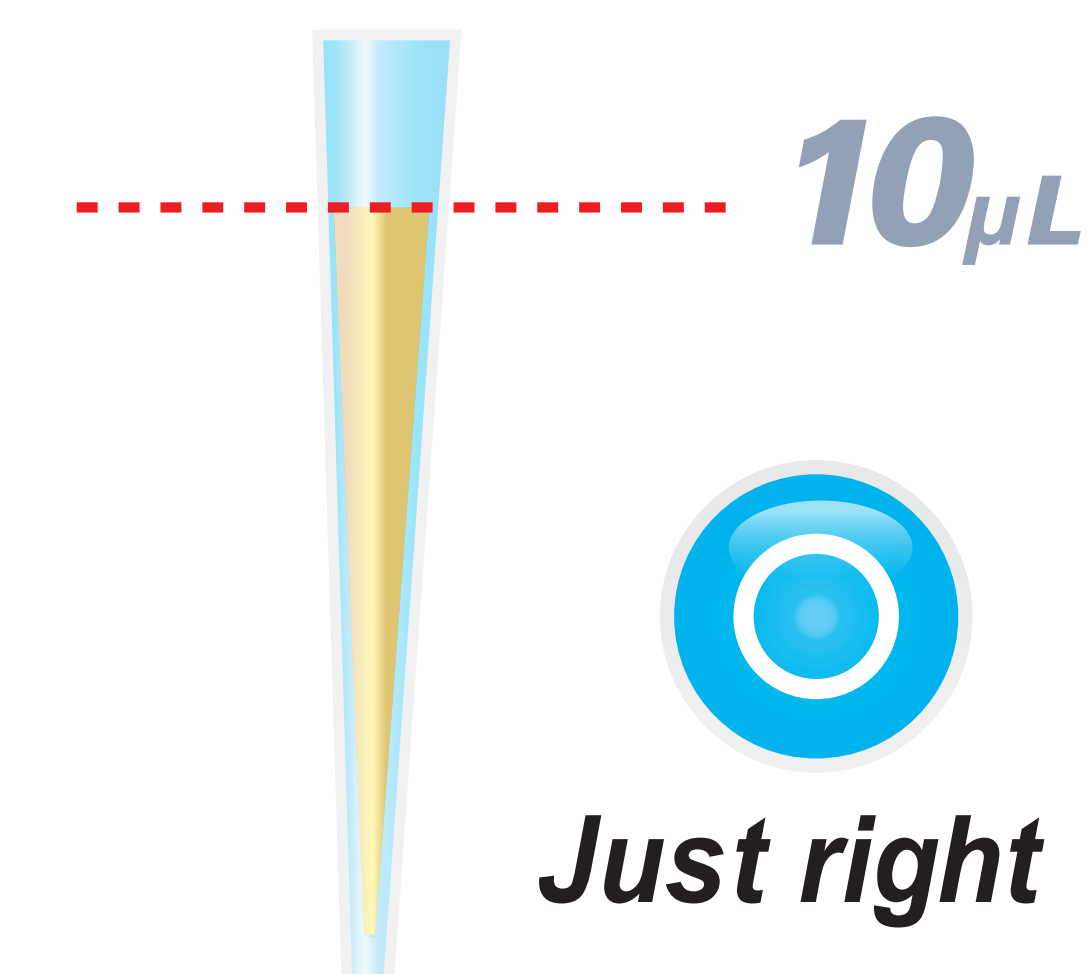


2 Add it into detection buffer tube




3 Shake the sample mixture tube

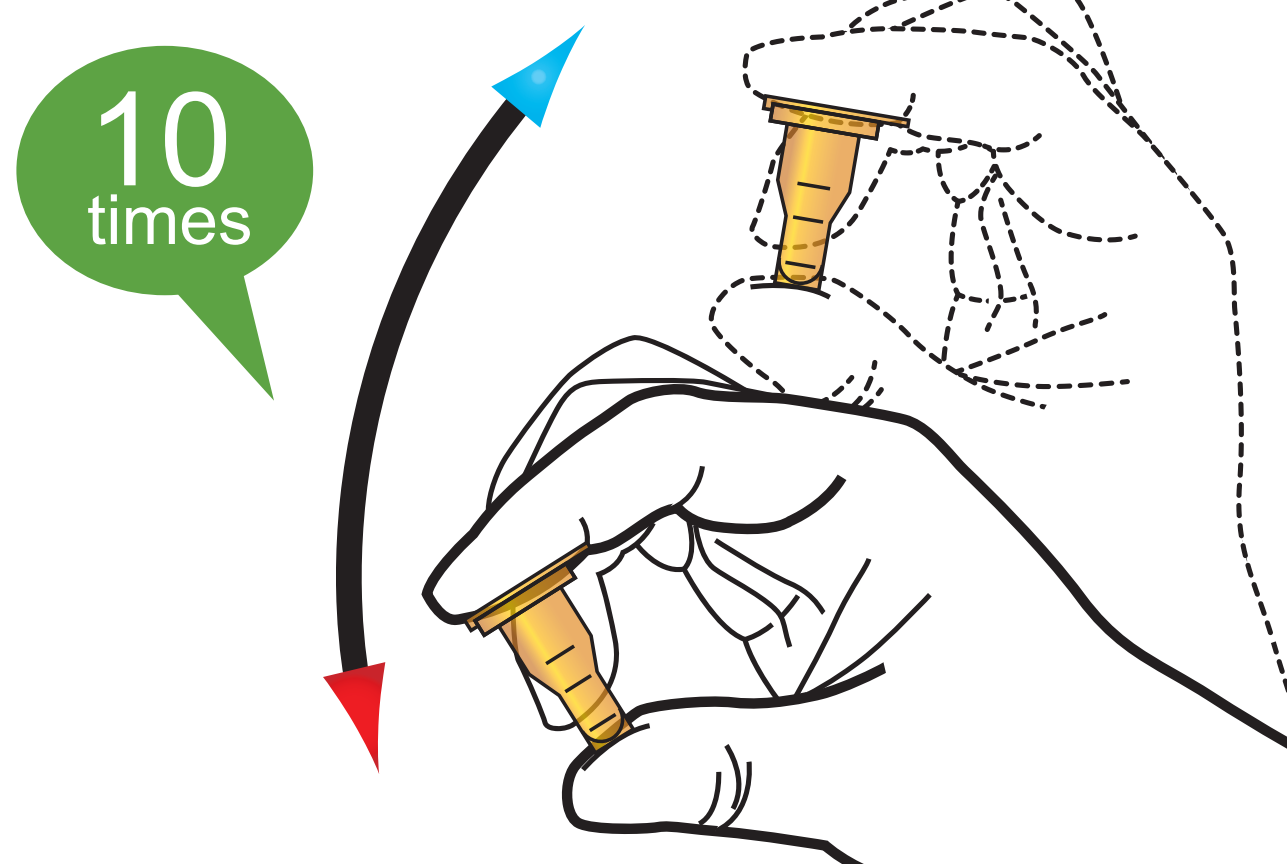

4 Draw the sample mixture

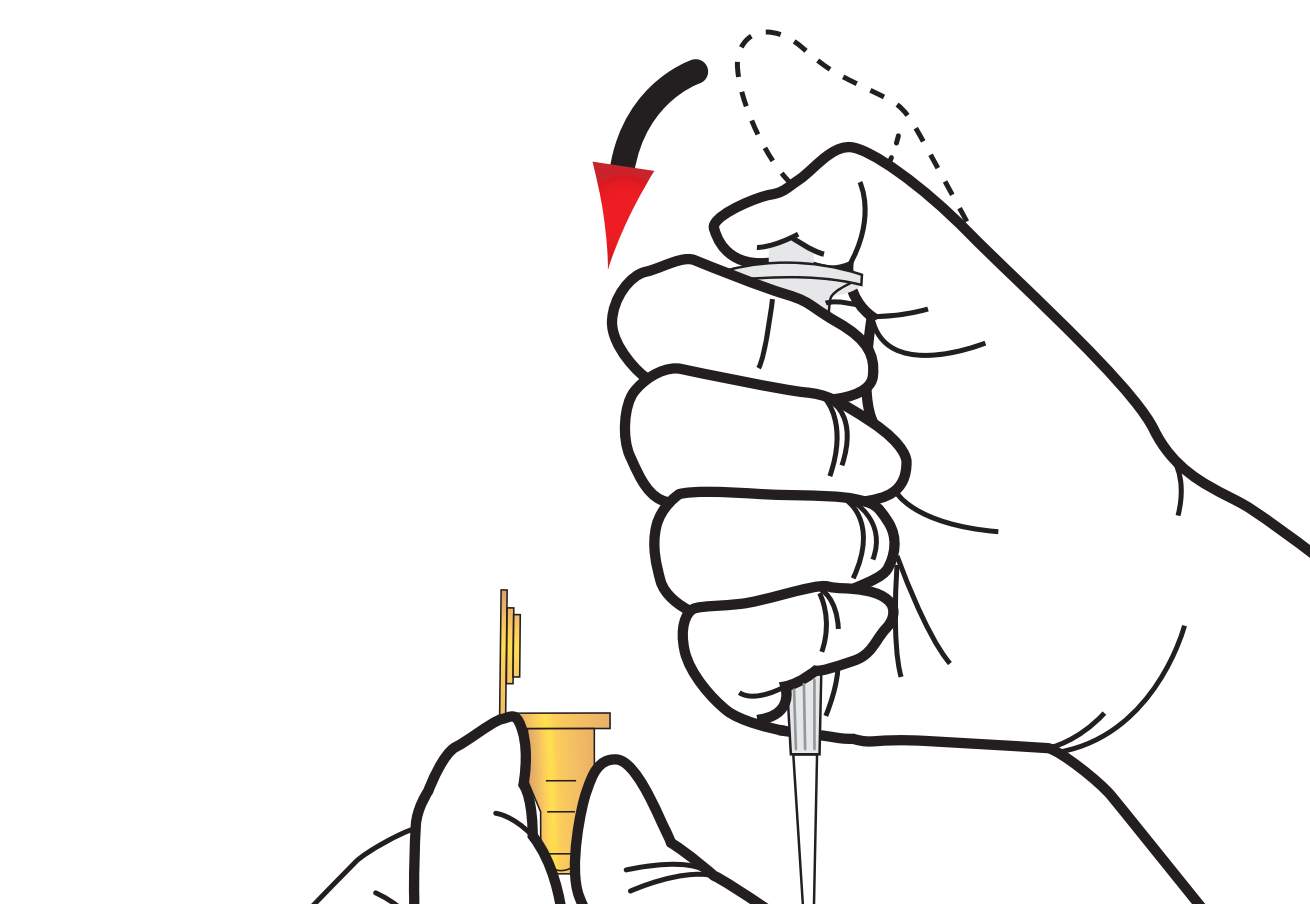


5 Load the sample mixture

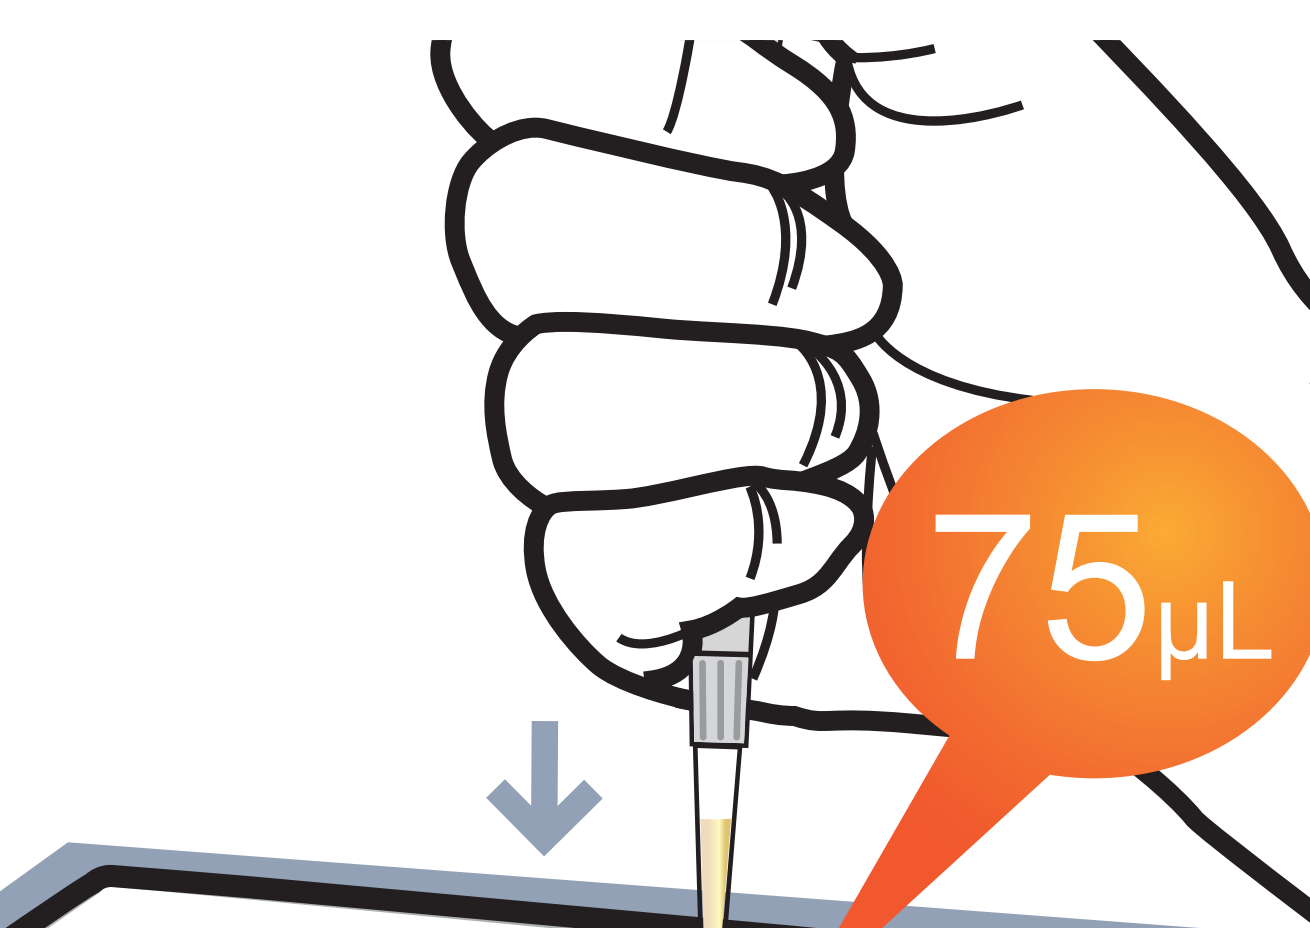


6 Waiting 10 minutes



7 Insert the test cartridge

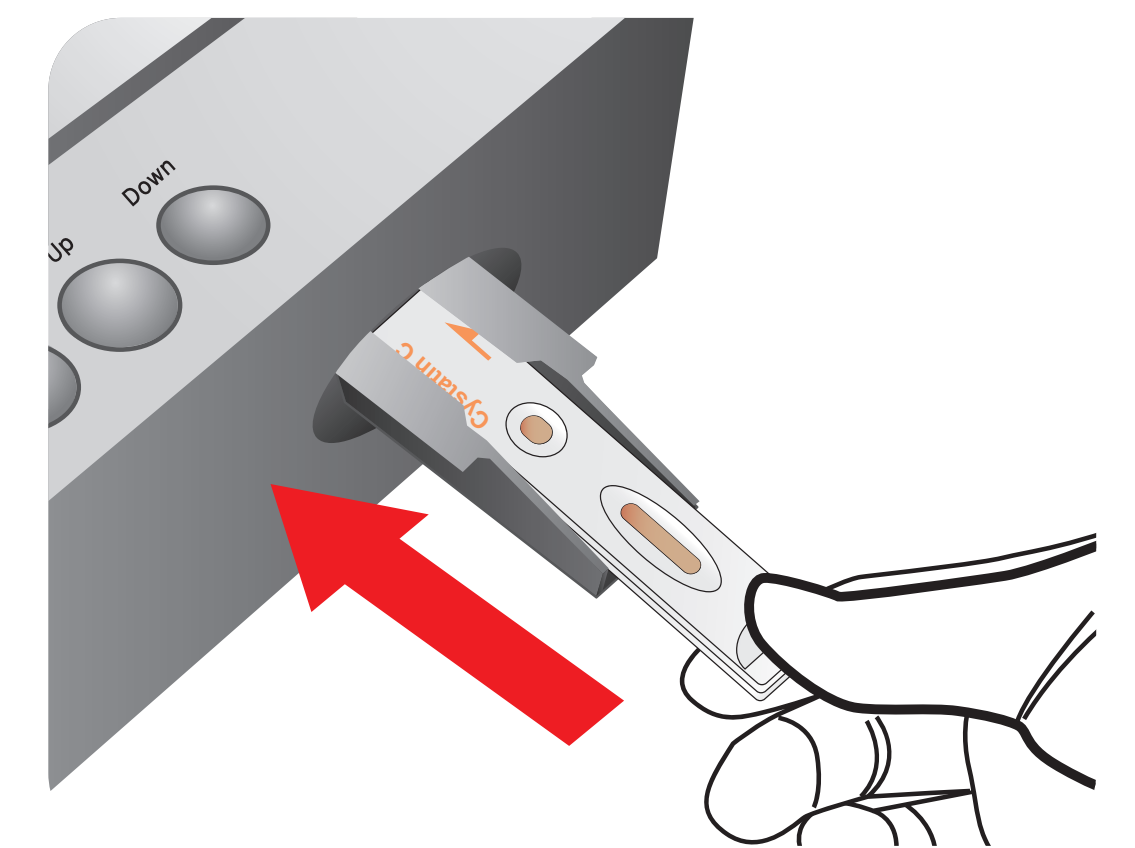

8 Press 'Select'

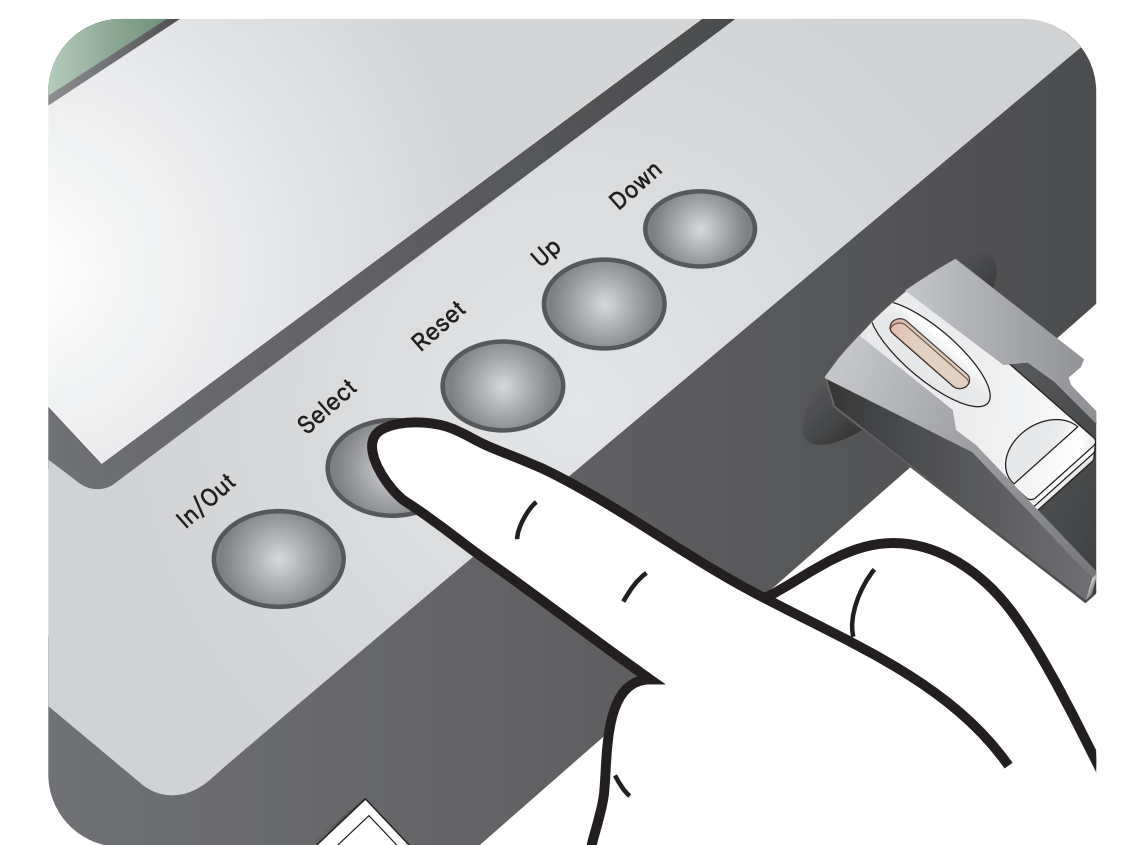

9 Read the test result

